

Supria
OPEN & COMPACT 16ch/32slice CT

#### **FUJ!FILM**

#### **FUJIFILM Healthcare Corporation**

9-7-3, Akasaka, Minato-ku, Tokyo 107-0052, Japan https://www.fujifilm.com/fhc/en

● "Supria", "Intelli IP", and "HiMAR" are registered trademarks or trademarks of FUJIFILM Healthcare Corporation in Japan and other countries. ● "DICOM" is the registered trademark or trademark of the National Electrical Manufacturers Association in the United States for its standards publications relating to digital communications of medical information. ● Specifications and external appearance are subject to change without prior notice. ● For proper use of the system, be sure to read the operating manual prior to placing it into service. ● This product is a CLASS 2 LASER PRODUCT.

FCP-E503P Printed in Japan 2022-07-XK-(F)

## "Supria" meets Healthcare Needs.

With the aging of society around the world, the demand for reducing the physical burden on patients is increasing at medical fields.

On the other hand, there is a demand for optimal and efficient hospital management, and it is also required to respond to various healthcare needs.

We will solve the challenges being faced in the medical practice with "Supria", which can meet the healthcare needs of present and future.


# 16ch/32slice



## "Supria" meets Patient Friendly


#### Iterative processing for routine examinations


To use the iterative processing (Intelli IP), a noise reduction technology, more efficiently on routine examinations, reconstruction speed has been improved by 50% compared to the Conventional CT.In addition, the intensity of noise reduction can be selected from seven levels, providing high quality images with appropriate exposure dose, image noise reduction and artifact reduction based on the operation guideline at clincal sites.

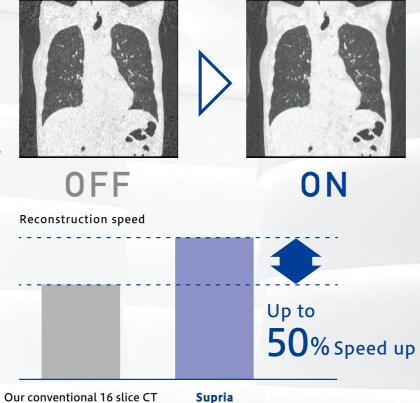


#### High throughput, high image quality

High performance, such as high-speed rotation, submillimeter slice imaging, powerful X-ray generator and state-of-the-art image reconstruction algorithms, realizes high resolution and high throughput examinations.

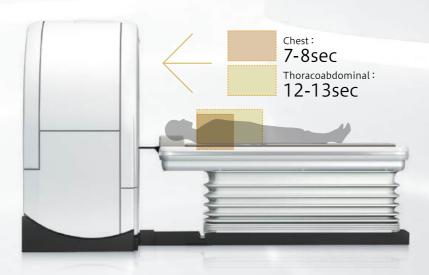

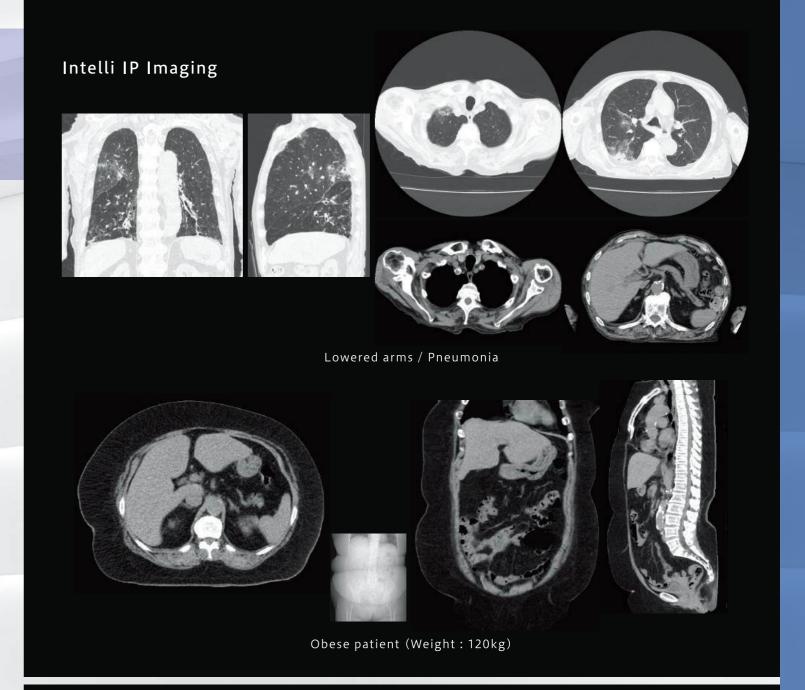

#### High-speed Scanning

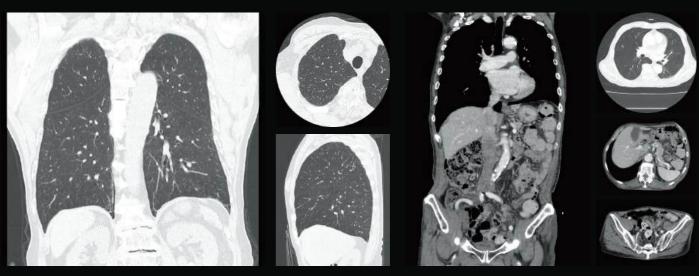

Chest scannig

Thoracoabdominal scanning


03

## "Supria" meets High Performance

#### Submillimeter slice imaging for high resolution and high quality images

Supria realizes high resolution images in a short time based on 0.625mm x 16ch scanning. In addition, high resolution and smooth 3D images and MPR images can be achieved by submillimeter slice scanning. Oblique images by MPR can be also achieved after scanning.






Before achieving Oblique image After achieving Oblique image

#### High quality imaging with the gantry tilt

The gantry has a function of tilting within a range of ± 30 degrees, which is possible to reduce exposure to highly radiation sensitive tissues.

In addition, excellent, high-quality images with low contrast can be achieved by normal scan of the head, compared to volume scan.

This imaging method takes into account exposure to the patient as well as image quality.






#### High efficiency powerful X-ray generator

Our technology enables to develop a powerful and high efficiency X-ray generator.


It achieves sufficient output with a compact power supply facility. It can also cover heavy load examinations on X-ray tube, such as wide-area imaging and multi-phase imaging.





#### Submillimeter slice imaging for high resolution and high quality images



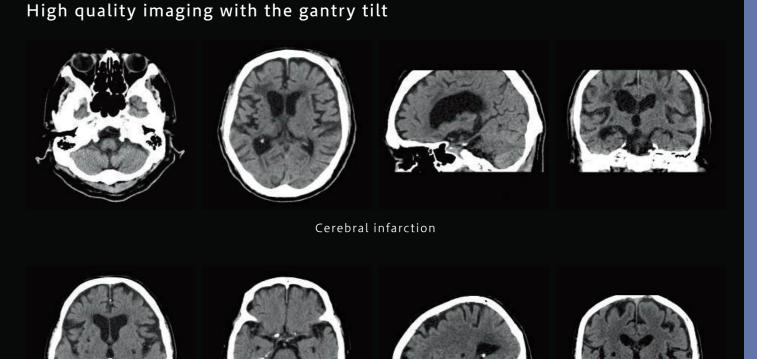


Lacunar infarction

# "Supria" meets High Functionality


#### HiMAR reduces metal artifacts

HiMAR (High Quality Metal Artifact Reduction) adopts unique algorithms for estimating and correcting artifacts based on metal data.

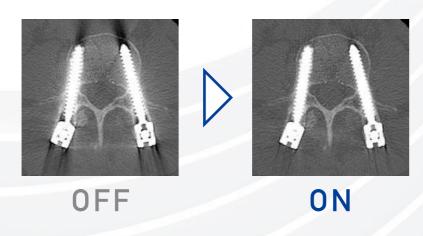

#### Capable of imaging in various patient's positions

With a large bore of 750mm and a maximum effective field of view that reduces anxiety of the patient, it is possible to scan with various patient's positions.

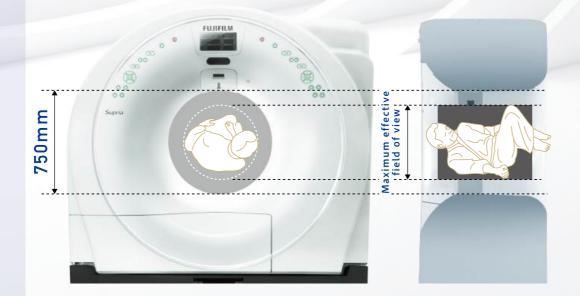


#### ECG Prospective scanning in synchronization with electrocardiogram

ECG Prospective scanning is a function that scans and achieves image in synchronization with electrocardiographic information. Images achieved by ECG Prospective scanning can be used for calcium scoring analysis\*.

\* A 3D workstation equipped with a calcium scoring analysis is required.

#### Helpful function to reduce the burden on the patient

Equipped with a motion artifact correction, body movement can be compensated even after scanning. Even if the patient is out of the effective field of view, such as a patient with a kyphosis, images can be reconstructed without re-scanning in case it is within the maximum effective field of view.

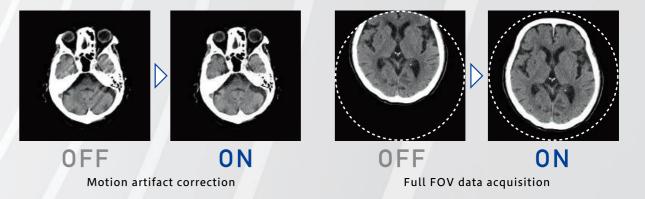

#### Intuitive operability with Quick Entry

The scan button is located on the intercom box, just above the keyboard, with simply arranged operation buttons, large text, and an easy-to-understand display, which support examinations efficiently.






3 Start!

Intercom box

07

## Clinical Images with Intelli IP







Head routine








Pulmonary emphysema




Breast cancer (suspected lymph node metastasis)

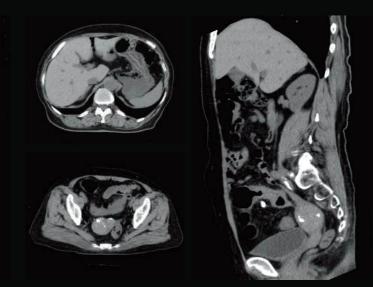

Uterine fibroids





Spondylolysis (10 years old )









Cuboid bone fracture



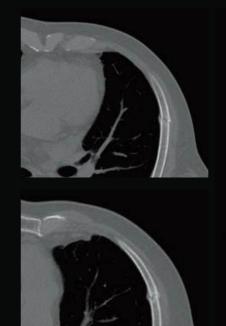










Rib fracture

Compression fracture


## Clinical Images with Intelli IP

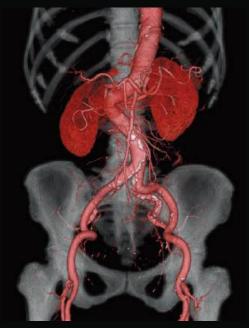


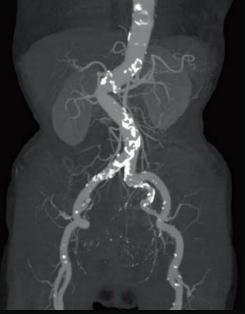



Abdominal CTA (100kV)
















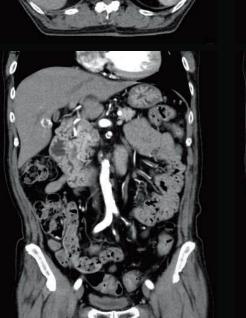












Hepatic hemangioma (Dynamic)

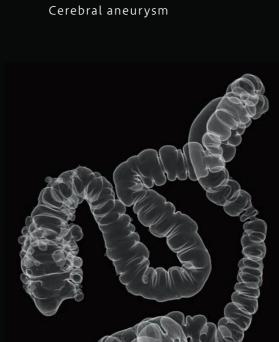








Colonic polyp




# "Supria" meets Comfortable Work Environment

#### Simple Dose Report

Dose information can be transferred to PACS as a secondary capture image. Using the PACS image viewer, the dose information can be checked together with the CT image.

#### **DICOM SR**

Using the DICOM standard, it is possible to transfer dose information

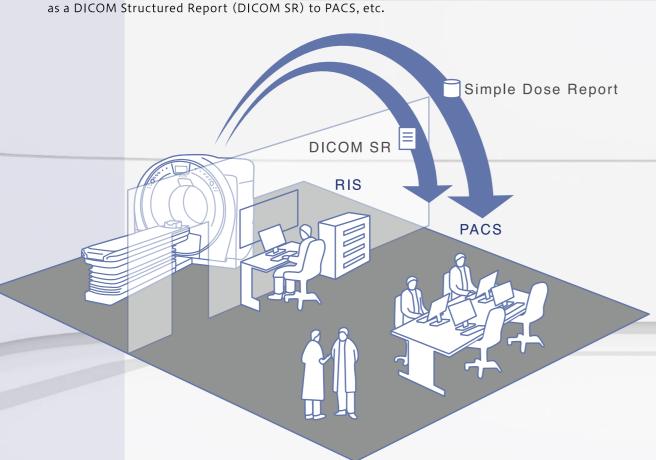

### Small footprint with 3-unit configuration


Only the gantry, the patient table, and the operation console configuration\* is realized. There are no other separate units with build-in system transformer, so the space in the CT room can be used effectively.

\* For power supply voltage 200V



#### Eco mode reduces stand-by power consumption

Supria is equipped with both On-time stand-by and Off-time mode function. With these Eco mode functions, it reduces power consumption of equipment in the gantry and energization time of the X-ray detector, thereby reducing power consumption during stand-by.

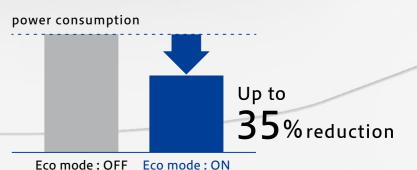

#### **Global Network**

We are committed to delivering advanced solutions,

including diagnostic imaging equipment that meets the needs of physicians and patients.

